

Алматы (7273)495-231
 Ангарт (3955)60-70-56
 Архангельск (8182)63-90-72
 Астрахань (8512)99-46-04
 Барнаул (3852)73-04-60
 Белгород (4722)40-23-64
 Благовещенск (4162)22-76-07
 Брянск (4832)59-03-52
 Владивосток (423)249-28-31
 Владикавказ (8672)28-90-48
 Владимир (4922) 49-43-18
 Волгоград (844)278-03-48
 Вологда (8172)26-41-59
 Воронеж (473)204-51-73
 Екатеринбург (343)384-55-89

Ижевск (3412)26-03-58
 Иваново (4932)77-34-06
 Иркутск (395)279-98-46
 Казань (843)206-01-48
 Калининград (4012)72-03-81
 Калуга (4842)92-23-67
 Кемерово (3842)65-04-62
 Киров (8332)68-02-04
 Коломна (4966)23-41-49
 Кострома (4942)77-07-48
 Краснодар (861)203-40-90
 Красноярск (391)204-63-61
 Курск (4712)77-13-04
 Курган (3522)50-90-47
 Липецк (4742)52-20-81

Киргизия (996)312-96-26-47

Магнитогорск (3519)55-03-13
 Москва (495)268-04-70
 Мурманск (8152)59-64-93
 Набережные Челны (8552)20-53-41
 Нижний Новгород (831)429-08-12
 Новокузнецк (3843)20-46-81
 Ноябрьск (3496)41-32-12
 Новосибирск (383)227-86-73
 Омск (3812)21-46-40
 Орел (4862)44-53-42
 Оренбург (3532)37-68-04
 Пенза (8412)22-31-16
 Петрозаводск (8142)55-98-37
 Псков (8112)59-10-37
 Пермь (342)205-81-47

Россия (495)268-04-70

Ростов-на-Дону (863)308-18-15
 Рязань (4912)46-61-64
 Самара (846)206-03-16
 Саратов (8342)22-96-24
 Санкт-Петербург (812)309-46-40
 Саратов (845)249-38-78
 Севастополь (8692)22-31-93
 Симферополь (3652)67-13-56
 Смоленск (4812)29-41-54
 Сочи (862)225-72-31
 Ставрополь (8652)20-65-13
 Сыктывкар (8212)25-95-17
 Сургут (3462)77-98-35
 Тамбов (4752)50-40-97
 Тверь (4822)63-31-35

Казахстан (772)734-952-31

Тольятти (8482)63-91-07
 Томск (3822)98-41-53
 Тула (4872)33-79-87
 Тюмень (3452)66-21-18
 Улан-Удэ (3012)59-97-51
 Ульяновск (8422)24-23-59
 Уфа (347)229-48-12
 Хабаровск (4212)92-98-04
 Чебоксары (8352)28-53-07
 Челябинск (351)202-03-61
 Череповец (8202)49-02-64
 Чита (3022)38-34-83
 Якутск (4112)23-90-97
 Ярославль (4852)69-52-93

<https://aptaca.nt-rt.ru> || acj@nt-rt.ru

Продукция для контроля стерилизации



STERILIZATION INDICATORS TAPES

Adhesive tape to indicate that sterilization process has been performed. Mono adhesive tape resistant to high temperatures and humidity, it has high adhesion on various types of fabrics, metals, plastics, no woven and papers. In accordance with ISO 11140-1(Class1).

Cod.	Length mt	Width mm	Sterilization type
5352	50	19	Steam
5355	50	25	Steam
5353	50	19	Dry heat, Poupinel method
5354	50	19	Ethylene Oxide Gas



GAS PLASMA CHEMICAL INDICATOR STRIP

The chemical process indicator strip gives visible confirmation, by colour change, that the item/pack has been exposed to Hydrogen Peroxide/Gas Plasma during processing in a Hydrogen Peroxide sterilizer and confirms the successfully penetration of the gas inside the pack. Packaged in a resealable aluminium bags of 250 pieces. In accordance to ISO 11140-1 (Class 3).

Cod.	Dim. mm
5370	14 x 97



BOWIE-DICK TEST

Bowie-Dick type test is a method to control periodically the correct autoclave function. This test allows to verify the air removal capacity and steam penetration for vacuum-assisted steamsterilizers process. The chemical indicator presents inside the disposable pack, ready to use, contains provided suitable spaces for the compilation, by the operator, of all the data relating to the test (date, operator, autoclave, result), which may then be filled, according to the regulations on force. In accordance with ISO 11140-1 (Class 2) and tested according to ISO 11140-4.

Cod.	Dim. mm
5380	130 x 100 x 17



STEAM INTEGRATOR

The chemical integrator SteriScan® indicator is a product that grants the correct steam sterilization parameters monitoring, both cycles at +134 °C and +121 °C. Very practical and precise, easy to read, inserted in the packs to be sterilized indicates whether the sterilization cycle happened correctly. Pack of 250 pieces in resealable laminate bag. In accordance with ISO 11140-1 (Class 5).

Cod.	Dim. mm
5390	20 x 101



ETHYLENE OXIDE GAS INTEGRATOR

The chemical gas integrator “CROSS CHECKS EO”, by check marks change color, has been designed to be used in ETO autoclaves for the correct sterilization process supervision. Pack of 250pcs in resealable laminated bag. Conform to ISO 11140-1 (Class 4).


Cod.	Dim. mm
5360	16 x 97



STERILIZATION PAPER

Medical crepe paper is manufactured according to EN 868 and ISO 11607-1. It is the ideal for materials packaging during the STEAM and ETO sterilization cycles. As barrier it provides excellent performances, it is damp-resistant and stable after the sterilization cycle. Weight: 60 gr/m² - Thickness: 0.160 mm. Green colour.

Cod.	Dim. cm
16903	50 x 50
16904	60 x 60
16907	90 x 90

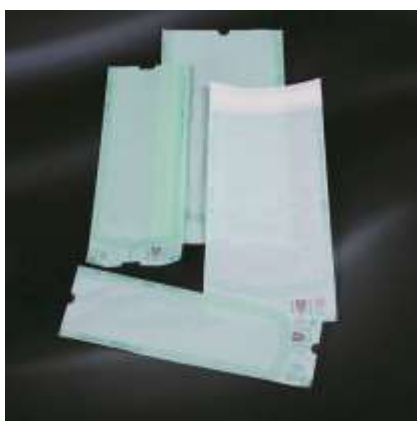


STERILIZATION POUCHES

Disposable flat pouches for surgical instruments or other Medical Devices sterilization, through EO Gas or Steam. Made in medical paper with transparent plastic film. On each pouch necessary data are printed to grant identification and traceability. There are also printed the irreversible radiating indicators for EO and Steam, whose colour variation indicates that the Device has undergone the sterilization process. Also available in self-sealing version with double-sides tape that allows the pouches closure as well in absence of sealing machine. Conform to UNI EN ISO 11607:1-2,

ISO 11140-1 and UNI EN 868-5 norms, classified as Class I Medical Devices, non sterile (93/42/CE).

Technical Data Sheet

Cod.	Type	Dim. mm
16710	Standard	75 x 250
16711	Standard	75 x 400
16712	Standard	100 x 250
16713	Standard	150 x 300
16714	Standard	300 x 500
16715	Self-sealing	90 x 230 x 40
16716	Self-sealing	130 x 250 x 40
16717	Self-sealing	190 x 330 x 40
16719	Self-sealing	300 x 450 x 40
16720	Self-sealing	300 x 500 x 40

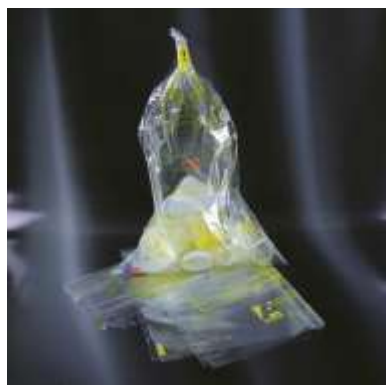


POLYPROPYLENE AUTOCLAVE BAGS

Polypropylene bags for autoclave sterilization, resistant up to 134°C. These bags are particularly useful in order to remove, by autoclave sterilization process, pathogenic substances normally present in contaminated containers (pipettes, specimen containers, test tubes, microtiter plates, petri dishes, etc.). Thickness 40 my.

Technical data sheet

Cod.	Dim. mm	Vol. lt
10570	300x660	15
10571	400x660	30
10572	600x760	80

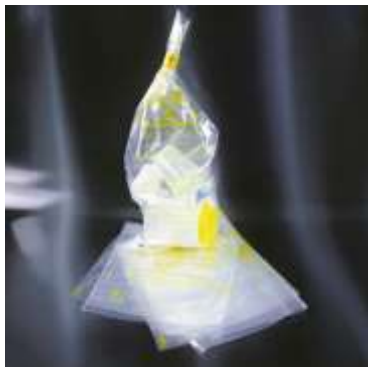

NYLON AUTOCLAVE BAGS

Nylon bags for autoclave or dry sterilization, resistant up to 180°C. These bags are particularly useful in order to remove, by autoclave or dry sterilization process, pathogenic substances normally present in contaminated containers (pipettes, specimen containers, test tubes, microtiter plates, petri dishes, etc.). Thickness 70 my.

Technical Data Sheet

Cod.	Dim. mm	Vol. lt
10580	300x660	15
10581	400x660	30
10582	600x760	80

Алматы (7273)495-231
Ангарск (3955)60-70-56
Архангельск (8182)63-90-72
Астрахань (8512)99-46-04
Барнаул (3852)73-04-60
Белгород (4722)40-23-64
Благовещенск (4162)22-76-07
Брянск (4832)59-03-52
Владивосток (423)249-28-31
Владикавказ (8672)28-90-48
Владимир (4922) 49-43-18
Волгоград (844)278-03-48
Вологда (8172)26-41-59
Воронеж (473)204-51-73
Екатеринбург (343)384-55-89

Ижевск (3412)26-03-58
Иваново (4932)77-34-06
Иркутск (395)279-98-46
Казань (843)206-01-48
Калининград (4012)72-03-81
Калуга (4842)92-23-67
Кемерово (3842)65-04-62
Киров (8332)68-02-04
Коломна (4966)23-41-49
Кострома (4942)77-07-48
Краснодар (861)203-40-90
Красноярск (391)204-63-61
Курск (4712)77-13-04
Курган (3522)50-90-47
Липецк (4742)52-20-81

Киргизия (996)312-96-26-47

Магнитогорск (3519)55-03-13
Москва (495)268-04-70
Мурманск (8152)59-64-93
Набережные Челны (8552)20-53-41
Нижний Новгород (831)429-08-12
Новокузнецк (3843)20-46-81
Ноябрьск (3496)41-32-12
Новосибирск (383)227-86-73
Омск (3812)21-46-40
Орел (4862)44-53-42
Оренбург (3532)37-68-04
Пенза (8412)22-31-16
Петрозаводск (8142)55-98-37
Псков (8112)59-10-37
Пермь (342)205-81-47

Россия (495)268-04-70

Ростов-на-Дону (863)308-18-15
Рязань (4912)46-61-64
Самара (846)206-03-16
Саранск (8342)22-96-24
Санкт-Петербург (812)309-46-40
Саратов (845)249-38-78
Севастополь (8692)22-31-93
Симферополь (3652)67-13-56
Смоленск (4812)29-41-54
Сочи (862)225-72-31
Ставрополь (8652)20-65-13
Сыктывкар (8212)25-95-17
Сургут (3462)77-98-35
Тамбов (4752)50-40-97
Тверь (4822)63-31-35

Казахстан (772)734-952-31

Тольяти (8482)63-91-07
Томск (3822)98-41-53
Тула (4872)33-79-87
Тюмень (3452)66-21-18
Улан-Удэ (3012)59-97-51
Ульяновск (8422)24-23-59
Уфа (347)229-48-12
Хабаровск (4212)92-98-04
Чебоксары (8352)28-53-07
Челябинск (351)202-03-61
Череповец (8202)49-02-64
Чита (3022)38-34-83
Якутск (4112)23-90-97
Ярославль (4852)69-52-93